

Detection of Drug Administration Behavior with Swallowing Sounds

Xiaolin Sang¹, Shin'ichi Warisawa^{1,2}, Hao Zhang¹, Katsumi Abe³, Masahiro Kubo³,
Kenichiro Tsuda³ and Ichiro Yamada^{1,2}

¹*School of Engineering, The University of Tokyo, 7-3-1 Hongo, Bunkyo-ku, Tokyo, Japan*

²*Graduate School of Frontier Sciences, The University of Tokyo, 5-1-5 Kashiwanoha, Kashiwa, Japan*

³*Green Platform Research Laboratories, NEC Corporation, 1753 Shimonumabe, Nakahara-ku, Kawasaki, Japan*

Keywords: Drug Administration, Wearable Sensing, Swallowing Sounds, Wavelet Transform, Classification.

Abstract: In recent years, chronic diseases have become the main causes of death around the world, and medication non-adherence among patients with chronic diseases is a common problem. A system for detecting drug administration behavior in daily life is strongly required. Currently, there is not a system for detecting this behavior by using wearable sensors. In this paper, we propose a wearable sensing method for detecting drug administration behavior in daily life by using swallowing sound, which is available and suitable for daily monitoring. To recognize the behavior from swallowing activities, a classification methodology using wavelet based features as feature vectors and artificial neural network as classifier is proposed. A high classification accuracy of 85.4% was achieved in classifying two swallowing activities of drinking water and taking a capsule with water. Furthermore, we also propose a compensation method for time-dependent change based on the frequency characteristics of swallowing sound.

1 INTRODUCTION

In recent years, the number of chronic diseases has been increasing, and these diseases have become the main causes of death around the world. Here, medication non-adherence is a common problem among patients with chronic diseases, which can be blamed on forgetfulness and the high cost of medicine. According to the World Health Organization, increasing the effectiveness of medication adherence intervention may have a far greater impact on health than any improvement in specific medical treatment (Sabaté, 2003). Feedback gained from monitoring patients' medication adherence by detecting drug administration behavior in daily life is expected to be important health-care information for physicians.

For this reason, some researchers and companies have been developing systems to detect drug administration behavior. For instance, a medicine-taking support system on a smartphone was developed to detect the behavior by judging whether a cup with sensors is picked up (Y. Tanabe, 2012).

An edible sensor system is being developed in order to electronically confirm medication adherence. The system consists of an edible sensor

attached to a capsule and a wearable health monitor. After the sensor is ingested together with the capsule, a wearable health monitor worn on the body records the information from the edible sensor (Au-Yeung, 2010).

With the development of wearable sensing technology, the automatic detection and recognition of some activities have been realized and applied to our daily lives. Detecting drug administration behavior from human activity by using wearable sensors can guarantee such behavior with less stress for patients.

In this research, we aimed to develop a system for detecting drug administration behavior by using wearable sensors. A wearable sensing system that is available and suitable to detect such behavior and a methodology for the detection will be introduced.

2 WEARABLE SENSING SYSTEM FOR DETECTING DRUG ADMINISTRATION BEHAVIOR

To detect drug administration behavior by using

wearable sensors, two possible ways are to analyze upper body motions (hands, arms, and neck) with accelerometer and gyroscope and to analyze swallowing activity by using internal body microphone or surface electromyography (EMG) (Amft, O., 2009; Klahn, M. S., 1999). Compared with analyzing upper body motions, analyzing swallowing activity has less related activities to classify.

Using internal body microphone and surface EMG are two widely used sensing methods for evaluating swallowing activities. In some researches, these two methods both can be used to differentiate between swallowing activities such as swallowing different drinks and foods with different mass (Sazonov, E. S, 2010; Ertekin, C., 1995). However, considering difference of swallowing water without/with capsules making different swallowing sounds, an internal body microphone, which can detect their swallowing sounds, is selected in our research..

Among various internal body microphones, a bone-conduction microphone was selected to record swallowing sounds for the following reasons. As Figure 1 shows, the microphone is integrated in an earphone-like sensor to record internal body sound easily by inserting it into the ear. Its high sensitivity makes it possible to record swallowing sounds with high quality. Additionally, the microphone consists of a microphone for internal body sound and one for outside sound in order to record internal body sound with little influence from environmental sound, making it suitable for daily monitoring.

In the meal-time related activity recognition using sounds from the bone-conduction microphone, a high accuracy of 87% was achieved for classifying drinking, eating hard food, eating soft food, and speaking (H. Zhang, 2011). Therefore, the possibility of classifying drinking and taking medicine as two kinds of swallowing sounds that can be detected is hypothesized and verified in the following.



Figure 1: Bone-conduction microphone.

3 SWALLOWING ACTIVITY CLASSIFICATION

In this section, a swallowing sound collection, the proposed classification methodology for swallowing activities, classification results, and discussion are introduced.

3.1 Swallowing Sound Collection

From 20 subjects, the swallowing sound signals of drinking water (10 ml and 20 ml) and taking a capsule with water (10 ml and 20 ml) were collected by using the bone-conduction microphone and a throat microphone as references, and then recorded simultaneously with an IC recorder at a sampling rate of 48 kHz as Figure 2 shows. The swallowing sounds collected were analyzed with Matlab.

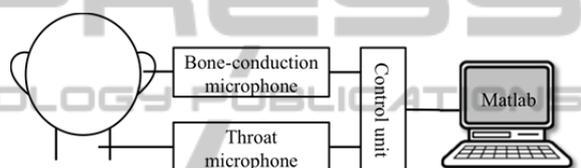


Figure 2: Swallowing sound collection system.

In the experiment, the substitute medicine is prepared by putting powdered foodstuff into the capsule shell. The subject drinks water that was prepared and takes capsules with water at his space. For each swallowing activity, five samples of sound signals were recorded.

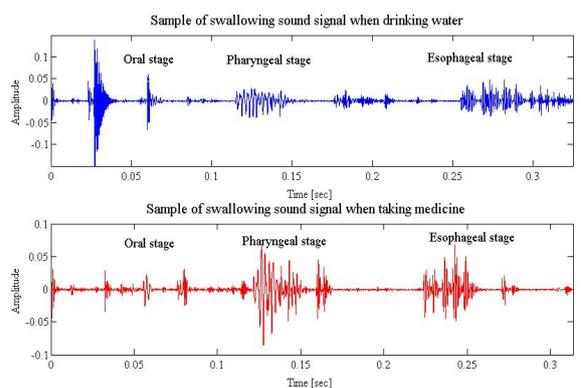


Figure 3: Swallowing sound signals when drinking water and taking medicine.

An example of swallowing sound signals when drinking and taking medicine is shown in Figure 3.

Swallowing sound is a non-stationary signal by nature and can be divided into stationary segments (Lazareck, L, 2002). About the components of

swallowing sound, it is said that three main components are respectively oral stage, pharyngeal stage and esophageal stage with respect to the position of bolus (Morinière, S, 2008).

From Figure 3, it is possible to differentiate drinking water and taking medicine using swallowing sounds.

3.2 Classification Methodology for Swallowing Activities

The proposed classification method of swallowing activities (drinking and taking medicine) can be divided into four stages: pre-processing, feature extraction, optimal feature selection, and classification.

After inputting a swallowing sound segment, the sound data is segmented and normalized. Then features are extracted, selected and used in the classification. Finally, whether the swallowing activity was drinking or taking medicine is output.

3.2.1 Pre-processing

In the classification, data in the pharyngeal phase is regarded as the target data. Raw signals are segmented to each swallowing sound segment and further segmented to the pharyngeal phase by comparing the envelope calculated from a Hilbert transform and the short-time energy of swallowing segments (20-ms frames with a 0.2-ms shifting). After the two-step segmentation, data in the pharyngeal phase is normalized linearly to reduce the individual differences and then resampled from 48 kHz to 4 kHz to obtain more detailed low-frequency information in feature extraction.

3.2.2 Feature Extraction

To differentiate the swallowing sounds made when drinking and taking medicine, a discrete wavelet transform is applied on data in the pharyngeal phase of swallowing sounds. With the decomposition, six levels of wavelet coefficients in different frequency ranges are obtained from the raw data, and statistical features (SF) and AR-model parameters of raw data and wavelet coefficients at each level are then extracted to represent the different characteristics of swallowing sounds made when drinking and taking medicine.

For the statistical features, six kinds of statistical features including maximum, mean, standard deviation, power, skewness, and kurtosis are

selected to characterize the wavelet coefficients at each level.

For the AR-model parameters, an autoregressive model (AR model) is used to forecast the variable of interest by using a line combination of the past values of the variables so that AR-model parameters are extracted to describe the waveforms by modelling time series information. The p -order AR model is defined as Equation 1.

$$y_t = c + \sigma_1 y_{t-1} + \sigma_2 y_{t-2} + \dots + \sigma_p y_{t-p} + e_t \quad (1)$$

where $\sigma_1, \sigma_2, \dots, \sigma_p$ are the AR-model parameters, c is a constant, and e_t is white noise.

In the feature extraction, the statistical features, the 7-order AR-model parameter at each wavelet level, and those from raw data are extracted separately to classify drinking and taking medicine (Figure 4).

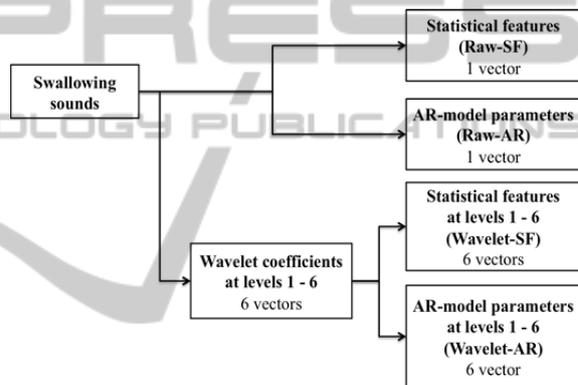


Figure 4: Feature extraction.

3.2.3 Feature Selection

For each subject, the statistical features or the AR-model parameters of a certain wavelet level were selected as the optimal feature vectors from the six levels of wavelet based features in Figure 4 depending on their performances for classification, because there exist large individual differences in swallowing sounds. Because there are only two target activities, to avoid the case that the classification accuracy of one activity becomes very large and that of the other activity becomes very low, we selected features not only regarding the average accuracy of the two activities but also considering the lower accuracy between them.

3.2.4 Classification

A neural network was selected as the classifier because of its high performance and little training time. In this research, a probabilistic neural network

(PNN) and an artificial neural network (ANN) were applied.

In the classification, because there exist large individual differences, the smoothing parameter in a PNN and the number of hidden layers in the structure of an ANN were adjusted to maximize the classification accuracy for each subject.

3.3 Classification Results

Leave-one-out cross validation was used to validate the performance of the method for classifying drinking and taking medicine, because it has an advantage of maximal use of data when the number of data is small. Figure 5 shows the average classification accuracies of drinking and taking medicine of 20 subjects with the raw data based features and the wavelet based features for the two classifiers.

From the comparison of the classification accuracies using different features and classifiers, the combination of wavelet based features and ANN classifier achieved the best performance (85.4%) for the classification of drinking and taking medicine.

Compared with the raw data based features, the wavelet based features proved to be more efficient at differentiating between drinking and taking medicine. ANN achieved more than 10% higher classification accuracy than PNN did.

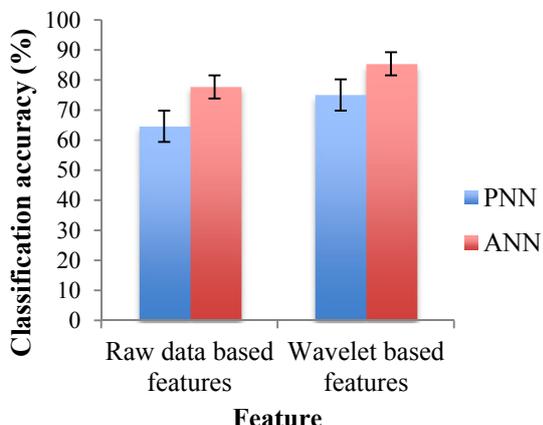


Figure 5: Comparison of classification methods.

The optimal feature selection for each subject is an efficient way to improve classification accuracy. For Wavelet-SF and Wavelet-AR, as the average classification accuracy of 20 subjects is shown in Figure 6 and Figure 7, the optimal level performed best. Because there exist large individual differences, the optimal level for classifying the two swallowing activities was different in individuals.

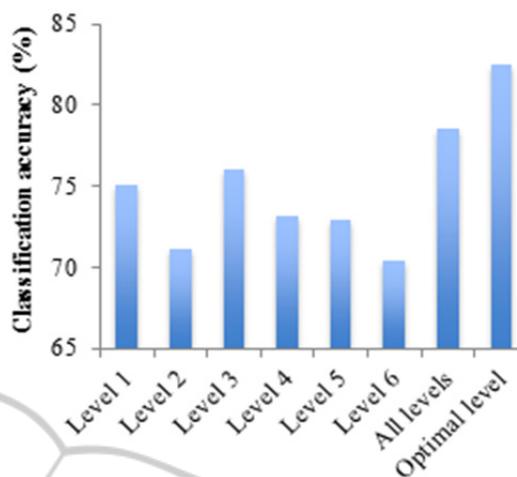


Figure 6: Comparison of classification results (average of 20 subjects) using Wavelet-SF of levels 1 - 6, all levels, and optimal level.

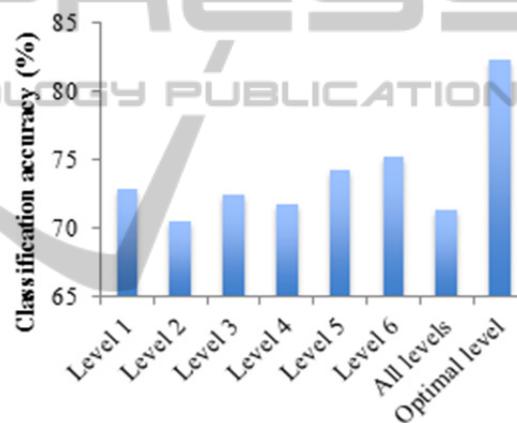


Figure 7: Comparison of classification results (average of 20 subjects) using Wavelet-AR of levels 1 - 6, all levels, and the optimal level.

The detailed average classification accuracy of 20 subjects is shown in Table 1. An average classification accuracy of 85.4% was achieved based on swallowing sound signals of 20 subjects. The classification accuracy of each subject ranges from 76.5% to 100%.

Table 1: Detailed classification accuracy (average of 20 subjects).

Activity	Drinking	Taking medicine	Overall
Average accuracy	85.0%	85.8%	85.4%

3.4 Discussion

The swallowing sound consists of the sound of bolus

flowing and that of throat movement with different frequency ranges. Differences between drinking and taking medicine possibly appear not only in the bolus flowing sound but also the throat movement sound. However, because of large individual differences, subject-dependent database is adopted in the classification and the most efficient frequency level is selected for each subject. Further, at the optimal frequency level, the statistical features such as amplitude and variance related features and the AR-model parameters for modelling time series also compute different characteristics. Hence, the optimal feature selection from the statistical features and the AR-model parameters at the six wavelet levels can maximize the classification accuracy for each subject.

PNN and ANN, used as two kinds of classifiers, were applied to classify drinking and taking medicine. The reason that PNN is not efficient in the classification of swallowing activities is that the number of samples is limited and not enough to train PNN.

4 VALIDATION OF TIME-DEPENDENT CHANGE

For the classification of drinking and taking medicine, a subject's specific database is adopted so that, in practical use, constructing a subject's specific database and training a neural network are necessary. For long-term use, the validation of time-dependent change is essential.

4.1 Validation Method and Experiments

We collected swallowing sounds made when drinking and taking medicine for three days with one-week intervals to validate whether time-dependent change exists in a short term.

The method for validating this change was designed in accordance with recognition in practical use. Data collected on the first day was regarded as a training set to select the optimal feature vector and to train a neural network, and data collected on the second and third days were used as a testing set.

4.2 Validation Results of Time-Dependent Change

Validation results for the time-dependent changes of three subjects are shown in Table 2, from which

time-dependent change can be ignored in a short term.

Table 2: Validation results for time-dependent change in a short term.

Subject	1st day	2nd day	3rd day
A	79%	74%	79%
B	77%	72%	82%
C	75%	71%	83%
D	81%	81%	75%

Furthermore, for Subject A, the time-dependent change based on six days of swallowing sound data taken over a one year interval was validated separately by using two optimal feature vectors, Wavelet-SF level 2 and Wavelet-AR level 5. As Figure 8 shows, time-dependent change in a long term can be ignored at level 2 (high frequencies) but exists at level 5 (low frequencies).

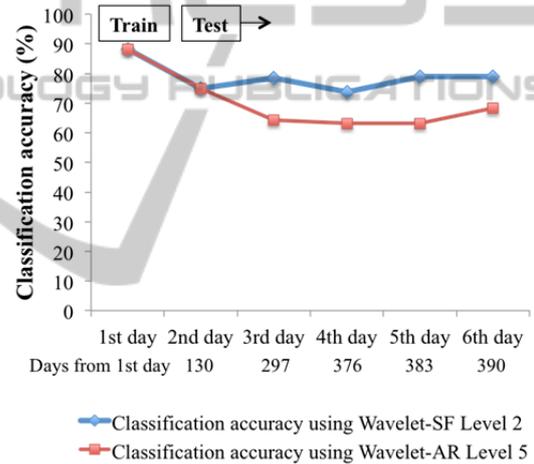


Figure 8: Validation results for time-dependent change in a long term for Subject A.

4.3 Discussion

The bolus flowing sound has frequency ranges corresponding to wavelet levels 1 to 4, and the throat movement sound has frequency ranges corresponding to wavelet levels 5 and 6.

To determine why testing results are reduced at the low frequency level (level 5), a sum of the absolute value of wavelet coefficients at each level defined as Equation 2 was calculated to describe the frequency characteristics of the swallowing sound of Subject A.

$$SWLC_m = \sum_{i=1}^{length} |y(i)| \quad (2)$$

where $SWLC$ represents the sum of the absolute value, y represents the wavelet coefficients or raw

data, m represents the wavelet level, and $length$ represents the length of the wavelet coefficients or raw data. After calculating $SWLC$ at each wavelet level, the ratio of $SWLC$ at each level to that of raw data is calculated as Equation 3.

$$Ratio_m = \frac{SWLC_m}{SWLC_{raw}} \quad (3)$$

The ratios of $SWLC$ at wavelet levels 1 - 4, which correspond to the frequency ranges of the bolus flowing sound, and those at wavelet levels 5 - 6, which correspond to the frequency ranges of the throat movement sound, are summed up separately to describe the characteristics of high frequencies and low frequencies, as shown in Table 3. The ratios of $SWLC$ in high frequencies to those in low frequencies on six days are also calculated as the last column in Table 3. As for the ratio of $SWLC$ in high frequencies to that in low frequencies, a large increase appears between the second and third days.

Table 3: Ratio of $SWLC$ in high frequencies and low frequencies.

Day	$SWLC$ in high frequencies (125 - 2000 Hz)	$SWLC$ in low frequencies (32 - 125 Hz)	Ratio of high to low
1st	17.50	1.09	16.0
2nd	18.47	1.12	16.5
3rd	16.20	0.77	21.1
4th	13.76	0.61	22.6
5th	13.93	0.70	19.9
6th	14.27	0.60	24.0

The ratio of the sum of the absolute values of wavelet coefficients in the high frequency ranges (levels 1 - 4) to that in the low frequency ranges (levels 5 - 6) can be considered as the change in swallowing sound as a possible reason for the time-dependent change in low frequency ranges.

4.4 Novel Proposal for Compensation for Time-dependent Change

On the basis of the acoustic characteristics of swallowing sounds, it is possible that throat movement sounds at low frequencies are affected easily by changes in a person's physical and mental conditions such as the state of throat movement. In comparison, the bolus flowing sound occurs by bolus flowing through the throat with little influence from a person's physical and mental conditions. Therefore, the bolus flowing sound at high frequencies is robust to time-dependent change, while some changes possibly occur in the throat movement sound over a long period of time.

Use of the bolus flowing sound is proposed to reduce time-dependent change. Therefore, the optimal feature selection from wavelet based features at high frequency levels (levels 1 - 4) can be regarded as a compensation method for time-dependent change.

5 CONCLUSIONS

In this research, an analysis method for detecting drug administration behavior by using swallowing sound was proposed, and a compensation method for time-dependent change based on the frequency characteristics of the sound was also proposed for long-term use.

In the classification of swallowing activities, a high classification accuracy of 85.4% was achieved by using the optimal feature vector from six levels of statistical features of wavelet coefficients and six levels of AR-model parameter of wavelet coefficients as features and an artificial neural network as a classifier. Due to the large individual differences, a subject-dependent database is adopted in the classification.

Generally, time-dependent change can be ignored in the classification of swallowing activities. However, for a long-term use, as a compensation method for time-dependent change, the use of wavelet based features at high frequency levels is proposed.

REFERENCES

- Sabaté, E. (Ed.), 2003. *Adherence to long-term therapies: evidence for action*. World Health Organization.
- Y. Tanabe, H. Takahashi, T. Tomii, Y. Iiduka and K. Yamasue, 2012. Design and an Experimental Evaluation of Training Data Management Method for Object-based ADL Recognition, *DEIM Forum 2012* C6-1.
- Au-Yeung, K. Y., Robertson, T., Hafezi, H., Moon, G., DiCarlo, L., Zdeblick, M., and Savage, G, 2010. A networked system for self-management of drug therapy and wellness. *Wireless Health 2010*. ACM, 2010, pages 1-9.
- Amft, O., Tröster, G., 2009. On-body sensing solutions for automatic dietary monitoring. *IEEE pervasive computing*. 8(2), pages 62-70.
- Klahn, M. S., Perlman, A. L., 1999. Temporal and durational patterns associating respiration and swallowing. *Dysphagia*, 14(3), pages 131-138.
- Sazonov, E. S., Makeyev, O., Schuckers, S., Lopez-Meyer, P., Melanson, E. L., and Neuman, M. R., 2010.

- Automatic detection of swallowing events by acoustical means for applications of monitoring of ingestive behavior. *Biomedical Engineering, IEEE Transactions on*, 57(3), 626-633.
- Ertekin, C., Pehlivan, M., Aydoğdu, I., Ertaşl, M., Uludağ, B., Çelebi, G., ... and Yüceyar, N., 1995. An electrophysiological investigation of deglutition in man. *Muscle & nerve*, 18(10), 1177-1186.
- H. Zhang, G. Lopez, M. Shuzo, J.J. Delaunay and I. Yamada., 2011. Analysis of Eating Habits Using sound information from a Bone-Conduction Sensor. *Proceedings of the IADIS International Conference 3-health 2011*.
- Lazareck, L., Moussavi, Z., 2002. Adaptive swallowing sound segmentation by variance dimension. In *Proc Eur Med Biol Eng Conf (EMBES)*.
- Morinière, S., Boiron, M., Alison, D., Makris, P., Beutter, P., 2008. Origin of the sound components during pharyngeal swallowing in normal subjects. *Dysphagia*, 23(3), pages 267-273.

SCITEPRESS
SCIENCE AND TECHNOLOGY PUBLICATIONS